




Aerosol protection using modified N95 respirator during upper gastrointestinal endoscopy: a randomized controlled trial

Chawisa Nampoolsuksan, Thawatchai Akaraviputh, Asada Methasate, Jirawat Swangsri, Atthaphorn Trakarnsanga, Chainarong Phalanusittheppha, Thammawat Parakonhthun, Voraboot Taweerutchana, Nicha Srisuworanan, Tharathorn Suwatthanarak, Thikhamporn Tawantanakorn, Varut Lohsiriwat, Vitoon Chinswangwatanakul

Department of Surgery, Faculty of Medicine Siriraj Hospital, Mahidol University, Bangkok, Thailand




Aerosol protection using modified N95 respirator during upper gastrointestinal endoscopy: a randomized controlled trial

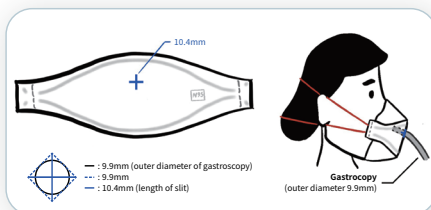

The standard N95 respirator (3M Aura 1870+ model) was modified to create a channel for endoscope insertion.

All patients aged 18 and above with undetectable COVID-19 virus who underwent diagnostic upper gastrointestinal endoscopy were enrolled and randomly assigned in 1:1 ratio into the modified N95 group and control (no mask) group.

The TSI AeroTrak (9306-04) handheld particle counter was used to measure the total number of particles. Particle sizes provided by the machine were ranged from 0.3, 0.5, 1, 3, 5, and 10 μm . The counter was placed at 1 meter away from patient during procedure.

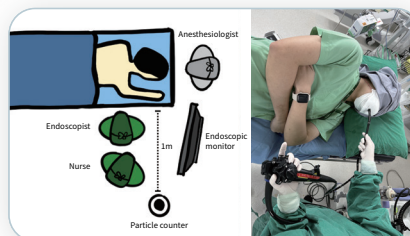

Results:

There was a statistically significant increase in 0.3- μm particle size in the control group compared to modified N95 group (242×10^3 counts/ m^3 vs. 68×10^3 counts/ m^3 , $p=0.045$). The amount of particle size over 0.3 μm was also higher in the control group.

No correlations between body mass index, choice of anesthesia, smoking, previous COVID-19 or respiratory tract disease, endoscopic duration, and the overall increased particle counts in both groups.

No adverse event was observed in both groups. The device did not cause any inconvenience for endoscopists and patients.

This modified N95 respirator had tendency to reduce particles, especially the particle size of 0.3- μm generated in upper gastrointestinal endoscopy

Clin Endosc 2024;57:335-341

Received: December 27, 2022 **Revised:** February 15, 2023

Accepted: February 22, 2023

Correspondence: Thawatchai Akaraviputh
 Department of Surgery, Faculty of Medicine Siriraj Hospital, Mahidol University, Bangkok 10700, Thailand
E-mail: akaraviputh@gmail.com

© This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/4.0/>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

Background/Aims: The coronavirus disease 2019 pandemic has affected the worldwide practice of upper gastrointestinal endoscopy. Here we designed a modified N95 respirator with a channel for endoscope insertion and evaluated its efficacy in upper gastrointestinal endoscopy.

Methods: Thirty patients scheduled for upper gastrointestinal endoscopy were randomized into the modified N95 ($n=15$) or control ($n=15$) group. The mask was placed on the patient after anesthesia administration and particles were counted every minute before (baseline) and during the procedure by a TSI AeroTrak particle counter (9306-04; TSI Inc.) and categorized by size (0.3, 0.5, 1, 3, 5, and 10 μm). Differences in particle counts between time points were recorded.

Results: During the procedure, the modified N95 group displayed significantly smaller overall particle sizes than the control group (median [interquartile range], 231 [54–385] vs. 579 [213–1,379] $\times 10^3/\text{m}^3$; $p=0.056$). However, the intervention group had a significant decrease in 0.3- μm particles (68 [–25 to 185] vs. 242 [72–588] $\times 10^3/\text{m}^3$; $p=0.045$). No adverse events occurred in either group. The device did not cause any inconvenience to the endoscopists or patients.

Conclusions: This modified N95 respirator reduced the number of particles, especially 0.3- μm particles, generated during upper gastrointestinal endoscopy.

Keywords: Aerosols; COVID-19; Endoscopy; Gastroscopy; N95 respirators

INTRODUCTION

Since the advent of the coronavirus disease 2019 (COVID-19) pandemic in 2019, upper gastrointestinal endoscopy has been considered an aerosol-generating procedure.^{1–3} Several studies have demonstrated the presence of the causative sudden acute respiratory syndrome coronavirus-2 virus in body fluids such as in oropharyngeal secretions. The viral infection is known to spread by aerosol particles $<5\ \mu\text{m}$ and droplets $>5\ \mu\text{m}$ in size.^{4–6} Endoscopic procedures have been adjusted to prevent human-to-human transmission.⁷ For treating patients with COVID-19, full personal protective equipment is mandatory for endoscopists and other healthcare personnel.^{8,9} However, some patients who test negative for COVID-19 before endoscopy may develop viral infection during the incubation period. Therefore, adequate protection of endoscopy personnel is required to prevent viral spread.

Various novel devices were developed to prevent viral dissemination during endoscopic procedures.^{10–15} An acrylic box was adapted for endotracheal intubation in COVID-19 patients to decrease the spillage of aerosols and droplets.¹⁶ The N95 respirator is a well-known and widely available mask that can filter at least 95% of 0.3- μm particles. Although COVID-19 viral particles are 0.125 μm in diameter, they are mostly adherent to body fluids. Since the N95 respirator can filter aerosols and droplets, thereby preventing viral transmission,¹⁷ here we modified the mask to enable endoscopic insertion and measured its efficacy for particle release during upper gastrointestinal endoscopy. We then assessed patient safety and endoscopist feedback.

METHODS

Study design

This study was conducted at the Siriraj Gastrointestinal Endoscopy Center (World Gastroenterology Organization-accredited training center), Faculty of Medicine, Siriraj Hospital, Mahidol University, Thailand.

Design of modified N95 respirator

A standard N95 respirator (3M Aura 1870+ model; 3M Health Care) was modified to create a channel for endoscopic insertion. In proportion to the 9.9-mm outer diameter of the gastroscope (GIF-HQ190; Olympus), two intersecting 10.4-mm linear puncture holes were created to fit the diameter of the scope to minimize aerosol spread during the procedure. A representative illustration of the modified N95 respirator is provided in Figure 1.

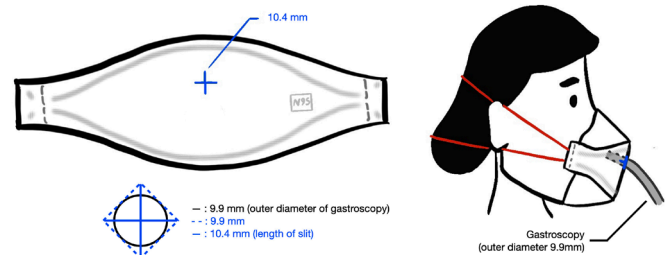


Fig. 1. Illustration of a modified N95 respirator. A standard N95 respirator (3M Aura 1870+ model) was modified as shown. In proportion to the 9.9-mm outer diameter of the gastroscope (GIF-HQ190; Olympus), two intersecting 10.4-mm linear holes were created and fitted to the diameter of the scope. Illustrated by the author.

Participants

All patients aged ≤ 18 years with undetectable COVID-19 on a nasopharyngeal swab tested by reverse transcriptase polymerase chain reaction within 48 hours of diagnostic upper gastrointestinal endoscopy were enrolled. Patients who required orotracheal intubation, required a transnasal endoscopy route, or had a previous history of upper gastrointestinal surgeries and unrelated procedures were excluded. All eligible patients were monitored during the procedure by an anesthesiologist.

Randomization and procedure

The participants were randomly assigned in a 1:1 ratio to the modified N95 or control group (no mask) using a computer-generated randomization program. Group allocation was performed by a nurse not involved in the procedure using sealed opaque envelopes. After allocation, each patient was transferred to the endoscopic unit and the endoscopic room was sealed to avoid unnecessary traffic that could interfere with particle counts during the procedure. Due to the nature of the intervention, the endoscopists and patients could not be blinded. All procedures were performed in one of two endoscopic rooms: A, room volume of 90 m^3 with an air flow change of 25 times/h, and B, room volume of 135 m^3 with an air flow change of 15 times/h. The endoscopists and other involved personnel wore surgical masks, gowns, disposable latex gloves, and closed-toe shoes or shoe covers throughout the procedure. All patients were placed in the left lateral decubitus position using supplemental oxygen via a nasal cannula. Anesthesia was chosen based on the anesthesiologist and patient's joint approval. For topical anesthesia before endoscopy, five puffs of 10% lidocaine were sprayed in the patient's mouth twice and retained for 10 seconds each time. A negative gag reflex was confirmed before the endoscopy commenced. For intravenous sedation, 25 to 75 $\mu\text{g/kg/min}$ of propofol and 1 $\mu\text{g/kg}$ of fentanyl were injected intravenously to achieve mild to moderate sedation as per the definition given in the American Society of Anesthesiologists guideline.¹⁸ After adequate anesthesia and oxygenation were ensured, a modified N95 respirator was placed over the patient's nose and mouth in the modified N95 group and an endoscope inserted through the channel. Endoscopic examinations were performed in both groups.

Outcome measurements

A TSI AeroTrak (9306-04) handheld particle counter (TSI Inc.) was used to determine the total number of particles (Fig. 2).

The counter has an acquisition flow rate of 2.83 L/min. Recorded particle sizes were 0.3, 0.5, 1, 3, 5, and 10 μm . The particle counter was placed 1 m away from the patient. The setup of the endoscopic unit is shown in Figure 3. Baseline particle counts were measured in the empty endoscopic room with closed doors for at least 15 minutes in the early morning before the first case of endoscopy that day. During each endoscopic examination, particle counts were measured and recorded every minute from the time of scope intubation to complete scope withdrawal. The primary outcome was the intergroup difference in particle counts during the procedures. The secondary outcomes were factors associated with increased particle counts and adverse events in patients wearing the modified N95 respirator. Feedback from patients and endoscopists was collected after every procedure. Patient demographic data, anesthetic techniques, and details of the upper gastrointestinal endoscopy were recorded.

Statistical analysis

Statistical analysis was performed using SPSS software ver. 18.0 (SPSS Inc.). Continuous variables are expressed as number (%) and mean \pm standard deviation for normally distributed variables and median with interquartile range (IQR) for non-normally distributed variables. The increased intergroup particle counts were compared using the Mann-Whitney *U*-test. Factors associated with changes in particle counts during the procedure were analyzed using bivariate correlations. Values of $p < 0.05$ were considered statistically significant.



Fig. 2. TSI AeroTrak (9306-04) handheld particle counter (TSI Inc.).

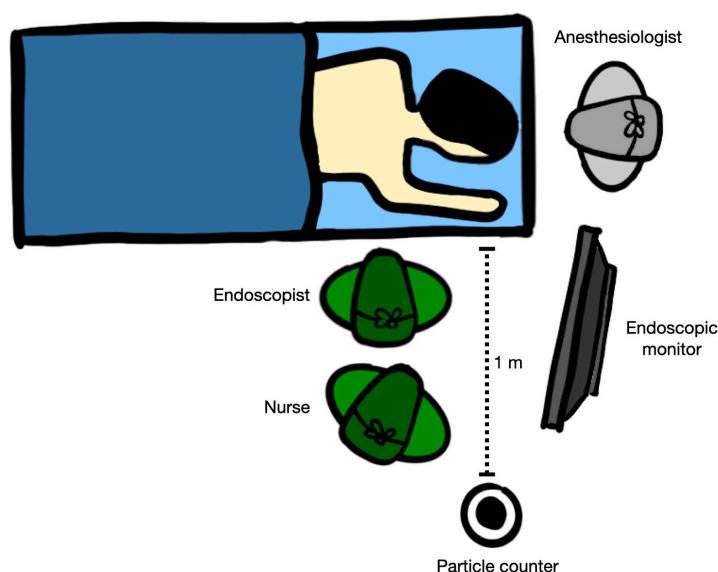


Fig. 3. Endoscopic unit setup. The TSI AeroTrak (9306-04; TSI Inc.) handheld particle counter was placed 1 m apart from patient at the same side as the endoscopist, without any blockages, and the endoscope was inserted through the modified N95 respirator. Illustrated by the author.

Ethical statements

This single-center randomized controlled study was approved by the Siriraj Institutional Review Board (approval number: Si-017/2022) and registered in the Thai Clinical Trials Registry (TCTR20220121006). Written informed consent was obtained from all participants.

RESULTS

Demographic data

The demographic data and endoscopic details of the N95 and control groups were comparable, including the nature of the disease and procedure time (Table 1). The baseline total particle counts of all particle sizes were also comparable between groups (358; IQR, 276–689 vs. 399; IQR, 288–753 $\times 10^3/\text{m}^3$; $p=0.279$).

Increased particle counts during endoscopic procedure

A statistically significant increase in 0.3- μm particle size was observed in the control group (242 vs. 68×10^3 counts/ m^3 ; $p=0.045$). The concentration of 0.3- μm particles was higher, but not statistically significant, in the control group. The control group had greater than two times the overall particles of the modified N95 group (Table 2).

Factors affecting increased particle counts

Our study found no correlation between the following factors: body mass index, choice of anesthesia, smoking, previous history of COVID-19 infection or respiratory tract disease, endoscopic duration, and overall increased particle count in either group (Table 3).

Adverse events

No complications were observed during or after the endoscopic examination in this study. Specifically, respiratory compromise or secretion obstruction were not observed in the modified N95 group during endoscope insertion. In addition, the endoscopists reported an absence of difficulty with endoscope insertion in the modified N95 group. All patients underwent one successful endoscope insertion attempt through the channel created in the modified N95 respirator.

DISCUSSION

Our study assessed the advantages and safety of using a modified N95 respirator for controlling aerosol dissemination in patients that undergo upper gastrointestinal endoscopy. The study demonstrated that our modified N95 respirator reduced

Table 1. Patients' demographic data and endoscopic details

Variable	Modified N95 (n=15)	No mask (n=15)	p-value
Age (yr)	63.9±12.6	60.4±16.6	0.697
Body mass index (kg/m ²)	23.9 (22.9–26.3)	24.9 (23.5–26.6)	0.414
Female	6 (40.0)	10 (66.7)	0.272
Anesthesia			0.056
Topical	0 (0)	4 (26.7)	
Total intravenous anesthesia	5 (33.3)	6 (40.0)	
Both	10 (66.7)	5 (33.3)	
Smoking	0 (0)	3 (20.0)	0.224
Previous coronavirus disease 2019 infection	0 (0)	2 (13.3)	0.483
History of lung cancer or tuberculosis	2 (13.3)	2 (13.3)	>0.999
Endoscopist			0.682
Staff	3 (20.0)	5 (33.3)	
Resident/fellow	12 (80.0)	10 (66.7)	
Endoscopic room			0.245
A	12 (80.0)	8 (53.3)	
B	3 (20.0)	7 (46.7)	
Endoscopic diagnosis: benign ^{a)}	15 (100.0)	12 (80.0)	0.224
Procedure time (min)	14 (10–20)	15 (11–22)	0.165
Add-on procedures ^{b)}	14 (93.3)	13 (86.7)	>0.999

Values are presented as mean±standard deviation, median (interquartile range), or number (%).

^{a)}A common diagnosis was benign disease: gastritis in 13 patients (43%), gastric ulcers in 3 (10%), intestinal metaplasia in 3 (10%), subepithelial lesions in 3 (10%), gastric polyps in 2 (7%), reflux esophagitis in 1 (3%), and normal in 2 (7%). ^{b)}Add-on procedures included a rapid urease test in 11 patients (37%), tissue biopsy in 3 (10%), and both in 13 (43%). Pathology reports of tissue biopsy included six of gastritis, six of gastric intestinal metaplasia, one of adenomatous polyp of the duodenal bulb, one of diffuse large B-cell lymphoma of the stomach, and one of squamous cell carcinoma of the upper esophagus.

Table 2. Increased particle count by study group

	Modified N95 (n=15)	No mask (n=15)	p-value
Overall particle (×10 ³ /m ³)	231 (54–385)	579 (213–1,379)	0.056
Particle size (×10 ³ /m ³)			
0.3 µm	68 (–25 to 185)	242 (72–588)	0.045
0.5 µm	85 (57–111)	213 (78–440)	0.067
1 µm	64 (37–84)	87 (47–408)	0.250
3 µm	23 (12–32)	31 (15–71)	0.325
5 µm	9 (5–14)	10 (3–26)	0.838
10 µm	1 (1–3)	3 (1–5)	0.345

Values are presented as median (interquartile range).

Table 3. Factors affecting increased particle count in both groups

Factors	r	p-value
Body mass index	0.188	0.320
Choice of anesthesia	0.155	0.412
Smoking	0.160	0.397
Previous coronavirus disease 2019 infection	0.232	0.218
Previous respiratory tract disease	0.272	0.146
Endoscopic time	0.087	0.647
Add-on procedure	–0.289	0.122

overall particle spillage by approximately 50% and significantly decreased 0.3-µm particle spillage by 72% versus patients who were unmasked during the endoscopic examination. This suggests that the transmission of COVID-19 viral particles that adhere to aerosols from body fluids can be prevented. Additionally, the respirator did not interfere with endoscopic examination or increase patient complications.

In the recent years of the COVID-19 pandemic, several innovations were proposed for aerosol and droplet prevention.^{10–15} A transparent acrylic box placed over the patient's head effectively reduced the spillage of droplets but interfered with the work of endoscopists.¹⁹ In addition, dental suction reduces the number of particles of all sizes that were detected during upper gastrointestinal endoscopy.^{20,21}

Topical anesthetic throat spray and coughing were strongly associated with maximal particle generation throughout upper gastrointestinal endoscopic procedures.^{22,23} In our study, we did not apply any suction devices, as this was not feasible in patients with masks. However, reflex coughing is blunted by intravenous sedation, as seen in patients of our study. It would be interesting to examine the beneficial effects of our respirator in

patients undergoing upper gastrointestinal endoscopy without sedation.

Owing to the insignificant intergroup difference in counts of particles $>0.3\ \mu\text{m}$, it is possible that the movement and activities of endoscopists and other healthcare personnel in the procedure room could have generated additional particle counts. The additional procedure, rapid urease test or biopsy, requires an additional instrument that is normally kept in a sealed package to avoid diffusion of dust into the air due to its unsealing. Moreover, larger particles can attach to droplets trapped within the mask or gravitate toward the ground before reaching the particle counter. In this study, the particle counter was kept 1 m apart from the patient's mouth as the distance between the patient's mouth and the endoscopist's nose was estimated to be approximately 1 m. Further, a shorter distance could have interfered with the endoscopic procedure.²⁴

The strength of this randomized study was the presence of a controlled environment (only two endoscopic rooms with limited traffic were used). Both staff and trainee endoscopists reported no difficulty during endoscopy in patients wearing masks, indicating that a modified N95 respirator could be effectively applied in daily practice. The original N95 respirator is widely available and the N95 respirator modification technique is simple, replicable at any hospital. The application of this modified N95 respirator is protective and practical for patients who may carry the risk of COVID-19 infection and present during their incubation period.

This single-center randomized study has some limitations. First, it included only uncomplicated upper gastrointestinal endoscopies. Therefore, the beneficial effect of respirators on particle reduction in advanced endoscopic interventions such as endoscopic retrograde cholangiopancreatography or endoscopic submucosal dissection should be established. Prolonged endoscopic duration, when multiple additional instruments are inserted through the working channel of the scope, may affect the capability of the mask. Second, the particle counter used to detect particle at 1 m in this study was limited to the detection of $0.3\text{-}\mu\text{m}$ particles. Different particle counters at variable distances may yield differing results. Finally, we used particle size as a surrogate marker for possible airborne viral spread. Whether particle reduction decreases the rate of airborne infection needs to be examined.

In conclusion, this study demonstrated that a modified N95 respirator could reduce the counts of the smallest (i.e., $0.3\text{-}\mu\text{m}$) particles and decrease the counts of larger particles. Therefore,

we conclude that the modified N95 respirator can be safely applied in patients requiring upper gastrointestinal endoscopy, without increasing procedural difficulty for the endoscopist.

Conflicts of Interest

The authors have no potential conflicts of interest.

Funding

None.

Acknowledgments

We thank Mr. Asadavudh Buachum and Miss Kanyanat Changpan from the Occupational Health Division for their cooperation with the particle measurements and Dr. Saowalak Hunnangkul for her assistance with the statistical analysis.

Author Contributions

Conceptualization: CN, TA; Data curation: CN, TA, TT; Formal analysis: CN, TA; Investigation: CN, TA, AM, TS; Methodology: CN, TA, VC; Project administration: CN, TA, JS, TP, TT; Resources: CN; Supervision: TA, VC, AM, VL; Validation: CN, TA, VL; Visualization: JS, AT, CP, TP, VT, NS; Writing—original draft: CN; Writing—review & editing: all authors.

ORCID

Chawisa Nampoolsuksan	https://orcid.org/0000-0002-5990-4704
Thawatchai Akaraviputh	https://orcid.org/0000-0003-2969-2648
Asada Methasate	https://orcid.org/0000-0002-8726-365X
Jirawat Swangsri	https://orcid.org/0000-0003-3721-1859
Atthaphorn Trakarnsanga	https://orcid.org/0000-0002-1980-7782
Chainarong Phalanusitthepha	https://orcid.org/0000-0003-0931-0091
Thammawat Parakonthon	https://orcid.org/0000-0002-2990-0649
Voraboot Taweerutchana	https://orcid.org/0000-0003-2475-7553
Nicha Srisuworanan	https://orcid.org/0000-0003-3079-9848
Tharathorn Suwatthanarak	https://orcid.org/0000-0002-5409-284X
Thikhamporn Tawantanakorn	https://orcid.org/0000-0001-8468-4347
Varut Lohsiriwat	https://orcid.org/0000-0002-2252-9509
Vitoon Chinswangwatanakul	https://orcid.org/0000-0001-9662-1669

REFERENCES

1. Tran K, Cimon K, Severn M, et al. Aerosol generating procedures and risk of transmission of acute respiratory infections to healthcare workers: a systematic review. *PLoS One* 2012;7:e35797.
2. Klompas M, Baker M, Rhee C. What is an aerosol-generating proce-

- ture? *JAMA Surg* 2021;156:113–114.
3. Rana SS. Risk of COVID-19 transmission during gastrointestinal endoscopy. *J Dig Endosc* 2020;11:27–30.
 4. Kutti-Sridharan G, Vegunta R, Vegunta R, et al. SARS-CoV2 in different body fluids, risks of transmission, and preventing COVID-19: a comprehensive evidence-based review. *Int J Prev Med* 2020;11:97.
 5. Peng L, Liu J, Xu W, et al. SARS-CoV-2 can be detected in urine, blood, anal swabs, and oropharyngeal swabs specimens. *J Med Virol* 2020;92:1676–1680.
 6. Sagami R, Nishikiori H, Sato T, et al. Aerosols produced by upper gastrointestinal endoscopy: a quantitative evaluation. *Am J Gastroenterol* 2021;116:202–205.
 7. Gralnek IM, Hassan C, Beilenhoff U, et al. ESGE and ESGENA position statement on gastrointestinal endoscopy and the COVID-19 pandemic. *Endoscopy* 2020;52:483–490.
 8. South African Gastroenterology Society (SAGES). SAGES position statement on endoscopy and PPE requirements during COVID-19 pandemic [Internet]. SAGES; 2020 [cited 2022 Jul 1]. Available from: https://www.sages.co.za/newsletter_SAGES/PPE_Requirements.pdf
 9. Kongkam P, Tiankanon K, Ratanalert S, et al. The practice of endoscopy during the COVID-19 pandemic: recommendations from the Thai Association for Gastrointestinal Endoscopy (TAGE) in collaboration with the Endoscopy Nurse Society (Thailand). *Siriraj Med J* 2020;72:283–286.
 10. Kitiyakara T, Kamalaporn P, Poolsombat A, et al. Leak-testing of an endoscopic aerosol box for preventing SARS-CoV-2 infection during upper gastrointestinal endoscopy. *Siriraj Med J* 2021;73:702–709.
 11. Sabbagh L, Huertas M, Preciado J, et al. New protection barrier for endoscopic procedures in the era of pandemic COVID-19. *VideoGIE* 2020;5:614–617.
 12. Lazaridis N, Skamnelos A, Murino A, et al. “Double-surgical-mask-with-slit” method: reducing exposure to aerosol generation at upper gastrointestinal endoscopy during the COVID-19 pandemic. *Endoscopy* 2020;52:928–929.
 13. Fujifilm. Fujifilm launches droplet-shielding Mouthpiece “B1” and Endoscope Cover “P1” [Internet]. Fujifilm; 2020 [cited 2022 Jan 22]. Available from: <https://www.fujifilm.com/jp/en/news/hq/5477>
 14. Kikuchi D, Ariyoshi D, Suzuki Y, et al. Possibility of new shielding device for upper gastrointestinal endoscopy. *Endosc Int Open* 2021;9:E1536–E1541.
 15. Gao Y, Xie J, Ye LS, et al. Negative-pressure isolation mask for endoscopic examination during the coronavirus disease 2019 pandemic: a randomized controlled trial. *Clin Transl Gastroenterol* 2021;12:e00314.
 16. Lai HY. Aerosol box 2020 [Internet]. 2020 [cited 2022 Jun 15]. Available from: <https://sites.google.com/view/aerosolbox/home?authuser=0>
 17. Bar-On YM, Flamholz A, Phillips R, et al. SARS-CoV-2 (COVID-19) by the numbers. *Elife* 2020;9:e57309.
 18. American Society of Anesthesiologists. Continuum of depth of sedation: definition of general anesthesia and levels of sedation/analgesia [Internet]. American Society of Anesthesiologists; 2019 [cited 2021 Dec 25]. Available from: <https://www.asahq.org/standards-and-guidelines/continuum-of-depth-of-sedation-definition-of-general-anesthesia-and-levels-of-sedationanalgesia>
 19. Sagami R, Nishikiori H, Sato T, et al. Endoscopic shield: barrier enclosure during the endoscopy to prevent aerosol droplets during the COVID-19 pandemic. *VideoGIE* 2020;5:445–448.
 20. Chan SM, Ma TW, Chong MK, et al. A proof of concept study: esophagogastroduodenoscopy is an aerosol-generating procedure and continuous oral suction during the procedure reduces the amount of aerosol generated. *Gastroenterology* 2020;159:1949–1951.e4.
 21. Nampoolsuksan C, Chinswangwatanakul V, Methasate A, et al. Management of aerosol generation during upper gastrointestinal endoscopy. *Clin Endosc* 2022;55:588–593.
 22. Phillips F, Crowley J, Warburton S, et al. Aerosol and droplet generation in upper and lower GI endoscopy: whole procedure and event-based analysis. *Gastrointest Endosc* 2022;96:603–611.
 23. Gregson FK, Shrimpton AJ, Hamilton F, et al. Identification of the source events for aerosol generation during oesophago-gastro-duodenoscopy. *Gut* 2022;71:871–878.
 24. Taweerutchana V, Suwatthanarak T, Methasate A, et al. Laparoscopic surgery produced less surgical smoke and contamination comparing with open surgery: the pilot study in fresh cadaveric experiment in COVID-19 pandemic. *BMC Surg* 2021;21:422.