


Supplementary Figure 1. Normalized volume reduction at 45 days in (A) individual active patients and (B) individual placebo patients.

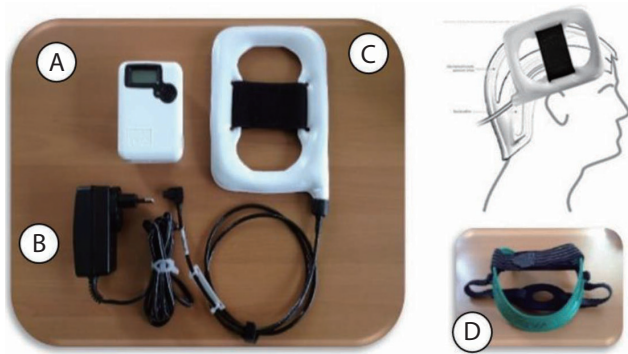

Supplementary Figure 2. I-NIC device. The figure shows the components of the I-NIC device: (A) generator, (B) power supply, (C) coil, and (D) helmet to keep the solenoid in place. pulsed electromagnetic field (PEMF) treatment was delivered for 5 consecutive days after stroke, for 2 hours every day.