


(A)

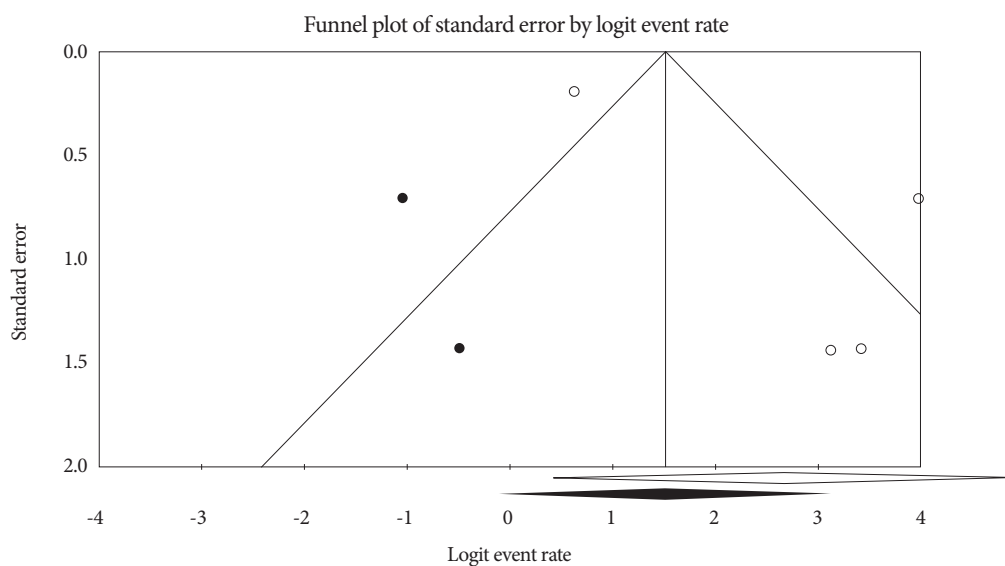

(B)

Supplementary Fig. 1. (A) Funnel plot of publication bias and Egger's regression test for included studies to assess adequacy of endoscopic ultrasound-guided liver biopsy. (B) Funnel plot of publication bias with Duval and Tweedie's trim and fill method.